


## **Specifications**

USAGE CONDITIONS		
Whole blood collection volume	450ml ± 50ml (excluding CPD: 63ml)	
Anticoagulant	CPD	
Whole blood holding time (prior to filtration)	At normal condition 2 to 24 hours after collection	At cool condition within 18 hours after collection
Holding temperature (prior to filtration)	Normal condition (~ 22° C)	Cool condition (~ 4° C)
Filtration temperature (during filtration)	Room temperature (~ 22° C)	
Filtration method	Gravity	
PERFORMANCE		
Residual WBCs	$<$ 1 x 10 $^{6}$ / bag with conformance 90 %	
RBC recovery	≥ 85 % (average)	
Residual hemoglobin	≥ 43g / bag	
Hemolysis	< 0.8 % at end of storage	
Filtration time	After holding at normal condition less than 30 min (average)	After holding at cool condition less than 1 hour (average)

### **Clinical Test**

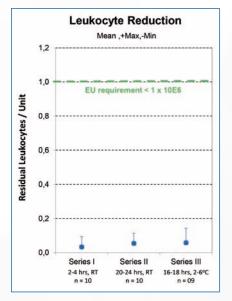





Source: Sanguin

#### For more information, please contact us:






Bionic Medizintechnik GmbH – a JMS corporation Max-Planck-Str. 21 · D-61381 Friedrichsdorf, Germany Telefon: +49(0)6172-75760 · Fax: +49(0)6172-757610 E-mail: info@bionic-jms.com · www.bionic-jms.com


THE BRIDGE TO GOOD HEALTHCARE



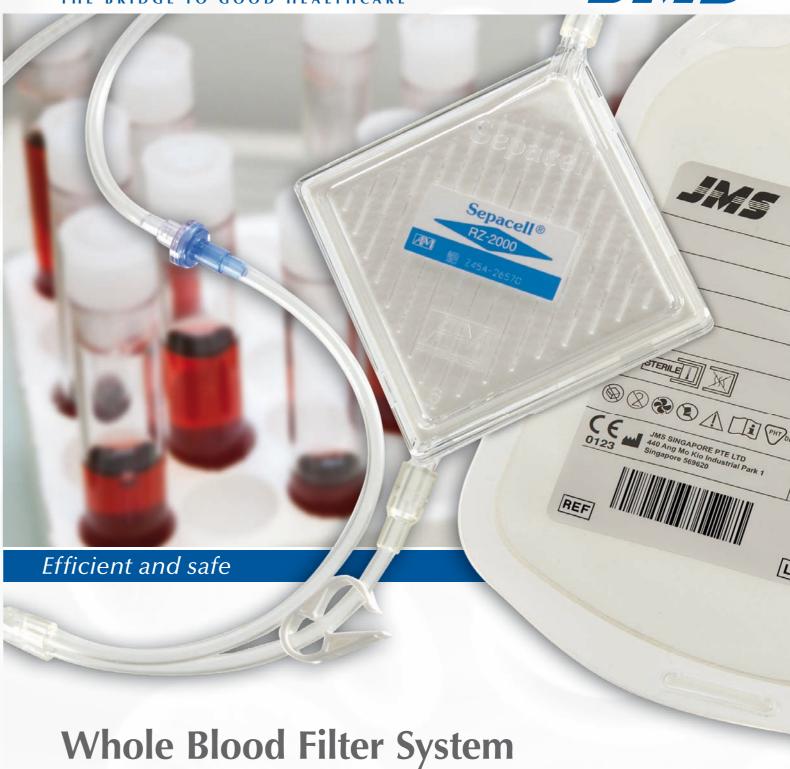


BLOOD BAGS WITH IN-LINE LEUKOCYTE FILTER

# **Whole Blood In-Line Filtration System**

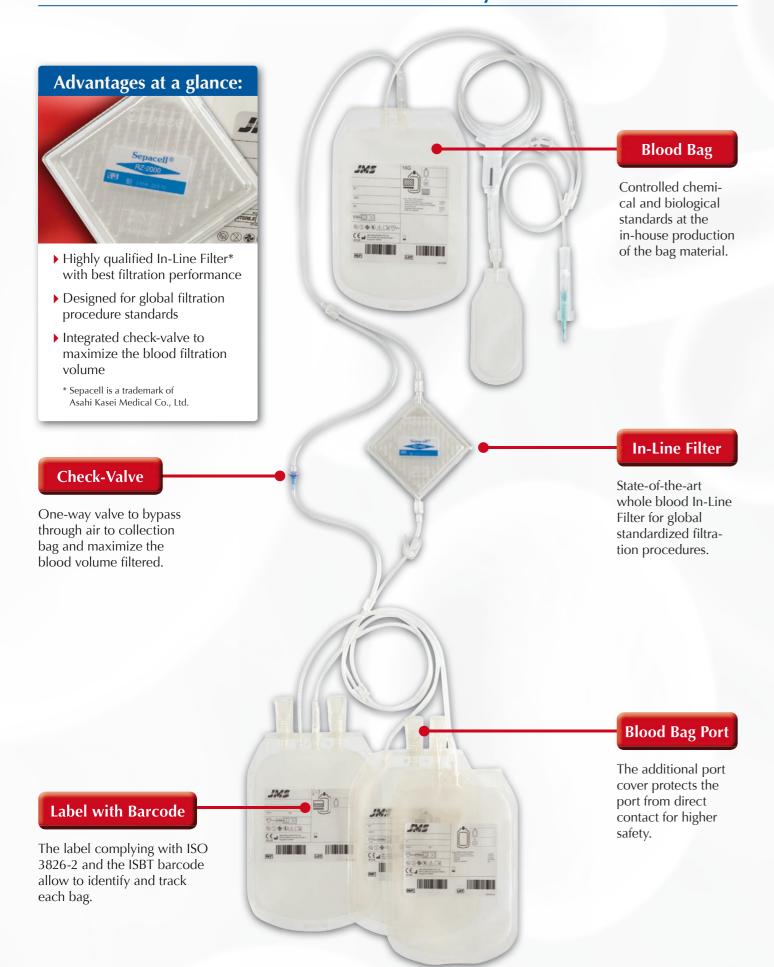


## **Filtration Procedure**




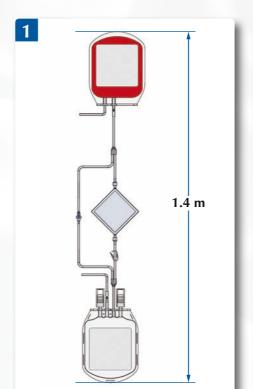


Place collection bag at a height of approximately 1.4 meter.

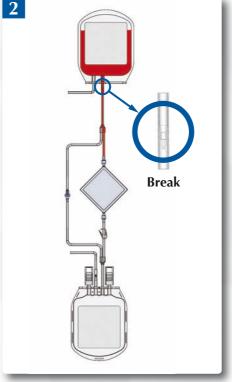


Break Snap Tip to allow the blood to flow into the filter.

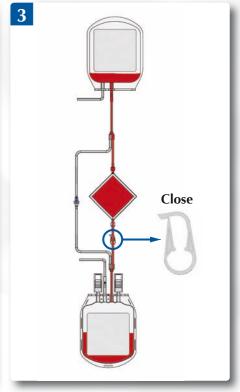


Close the clamp when 10% blood are still in the collection bag.

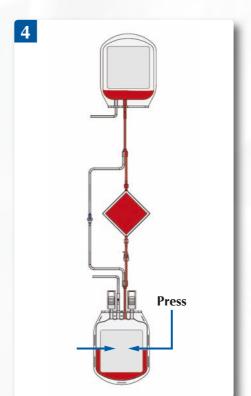

Press the lower bag to remove excess air through the check-valve.

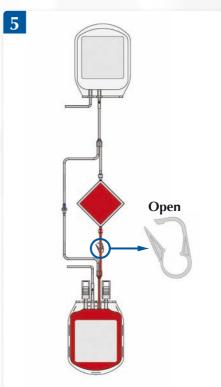

Open the clamp after excess air has been moved into collection bag.

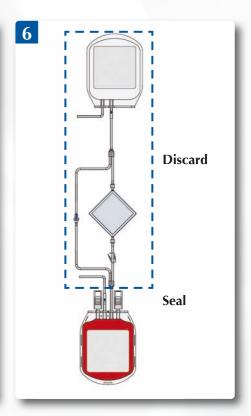

Complete filtration and seal-off tubing to discard collection bag and filter.